


New **ISO** Water Quality Standard for Hemodialysis

ISO 13959:2009



We See the Future Of Dialysis Water... **Today**

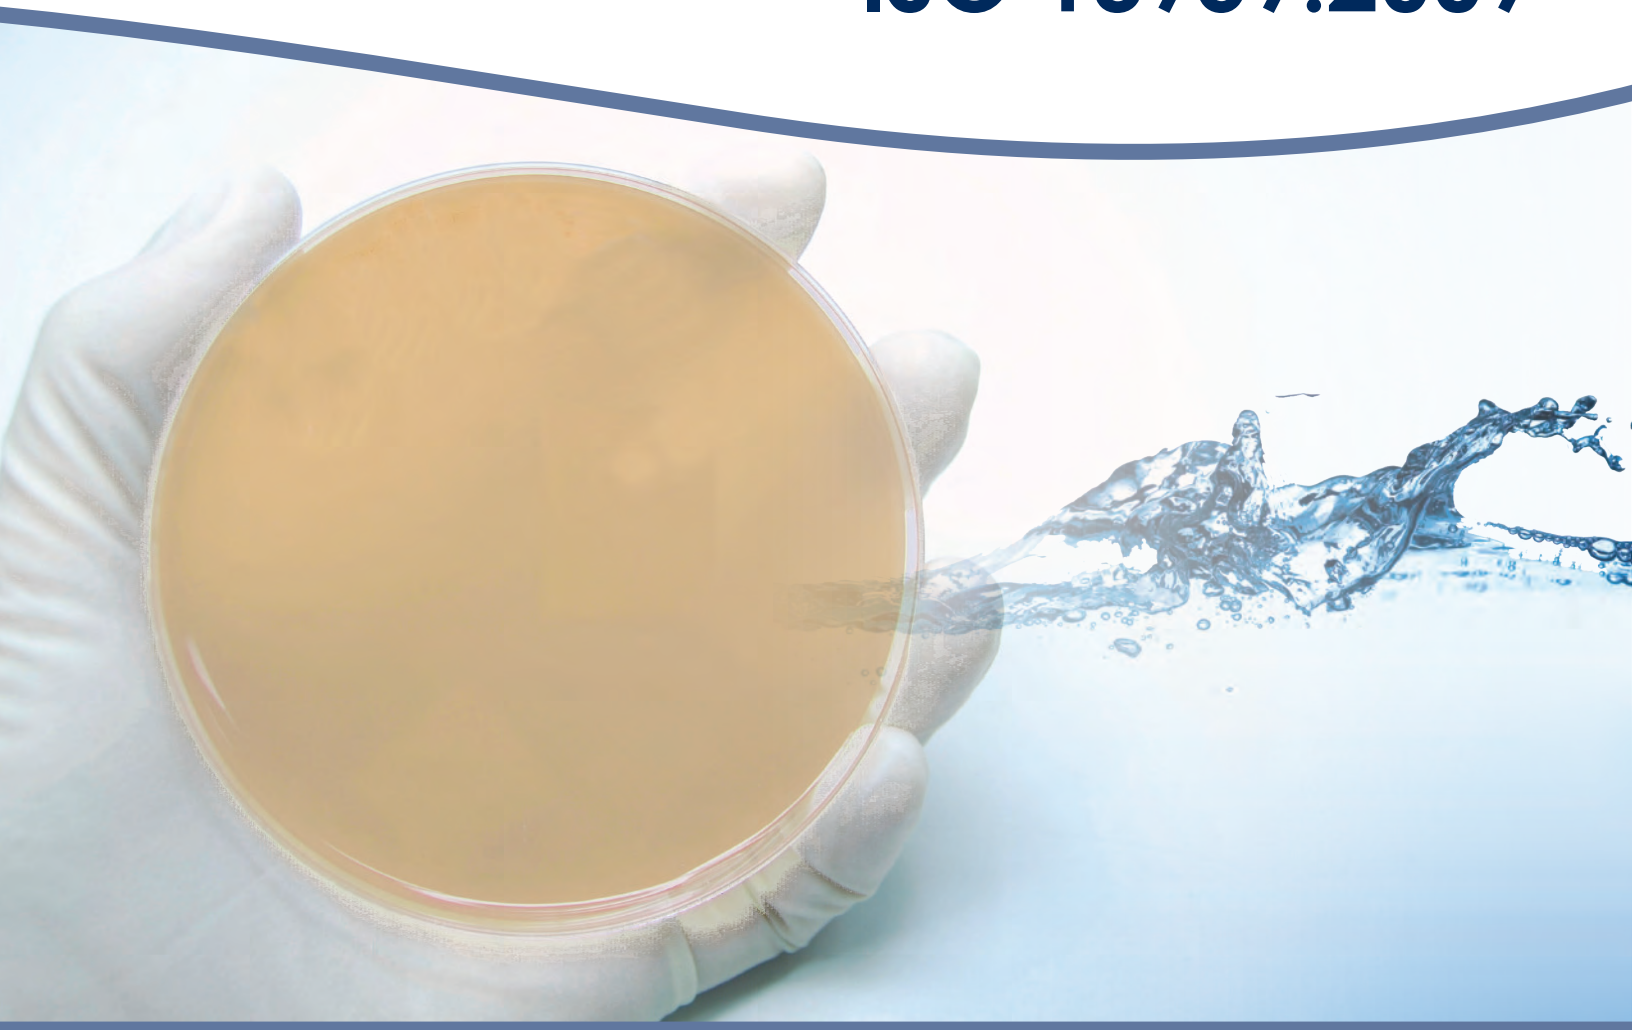

MAR COR[®]
PURIFICATION

A Cantel Medical Company

ISO 13959:2009

A New Water Quality Standard for Better Patient Outcomes

The recent adoption of ISO 13959:2009 by AAMI means the quality of water used in dialysis treatment will increase. The new standard has 2 important aspects to it. First, acceptable microbiological levels have been reduced by more than 50%, as noted in the chart below. Second, the testing protocol used to determine bacteria levels is a much more sensitive cultivation technique. The net result is that existing water system designs may or may not consistently produce water that meets the new standards.

AAMI Microbiological Standards for Dialysis Water

Microbiological Level	Previous Standards	New Standards	Previous Action Level	New Action Level
Colony Forming Units	< 200 CFU/mL	< 100 CFU/mL	≥ 100 CFU/mL	≥ 50 CFU/mL
Endotoxin Units	< 2 EU/mL	< 0.25 EU/mL	≥ 1 EU/mL	≥ 0.125 EU/mL





Microbiological Testing Procedure

In an effort to harmonize procedures for measuring microbiological levels in dialysis water, the new ISO standard defines the cultivation technique more precisely. The most important aspect is that the procedure provides growth conditions that favor microorganisms that thrive in water.

There are 3 main elements of the procedure: Agar medium, incubation temperature and incubation time. In many cases, the clinic does not perform the procedure but sends the samples to a certified laboratory for processing. These laboratories will be adopting the new standard.

Agar Medium: The 2 approved agars are Tryptone Glucose Extract Agar (TGEA) and Reasoner's Agar No. 2 (R2A). Both of these do well with water born microorganisms. This replaces the most commonly used agar, TSA.

Incubation Temperature: The incubation temperature was changed to mirror the actual water environment. Water temperatures are normally between 15-25°C, not at the current 35°C. Therefore, the new standard requires the temperature to be maintained between 17-23°C.

Incubation Time: In order to give the microorganisms time to develop, it has been determined that 7 days provides an accurate indication of viable bacteria. Many water systems are not disinfected during this time period so bacteria have an opportunity to grow. The current incubation time & temperature is 48 hours at 35°C and will be changed to 7 days at 17-23°C.

Results: These new cultivation conditions simulate the dialysis water environment and have been demonstrated to produce higher levels of bacteria as compared to the previous conditions. Although higher levels of bacteria are expected, some testing has shown little difference between the old and new conditions.

ISO 13959:2009 Water Quality Standard

What Can You Do?

For existing water systems, you should perform testing using the new ISO standard to ensure that your water system is producing water that meets the new requirements. As a result, you may need to increase the disinfection frequency, or add additional filtration or a combination of both in order to meet the new standard. Mar Cor Purification can help you evaluate the options.

For those considering new water systems, the use of heat for daily disinfection of the water distribution loop has been proven to be a state of the art design to minimize bacteria growth. The CWP central and WRO 300 H portable Reverse Osmosis Systems are designed for daily heat disinfection. The use of endotoxin retentive filters can also provide a level of safety for the water system.

If you have any questions about the new ISO Standard or what can be done to improve your water system's compliance to the standard, a Mar Cor Purification representative is available to help. Mar Cor Purification will be happy to meet with you to review your existing water system and to discuss options for any future water system design. Call us at 1-800-633-3080 or visit us on the web at www.mcpur.com.

Mar Cor Purification Medical Products & Services



Medical Water Systems

Mar Cor Purification is one of the largest and most experienced water purification suppliers to the Medical/Hemodialysis market. Mar Cor Purification has the largest equipment and service offerings and provides complete, installed, medical device registered water systems throughout North America. Each system is serviced from one of our nationwide service offices, which are stocked with critical medical device spare parts.



Medical Water Products

Mar Cor Purification offers a wide variety of medical water products and services, in addition to water systems, to ensure that hemodialysis clinics and their employees have the equipment, products, information, and service to effectively provide their patients with the highest quality water available. From product support, to essential parts, to ongoing education, We have the resources to keep your water treatment system and clinic running smoothly.



Medical Water Services

Mar Cor Purification is one of the largest and most experienced water purification companies in North America. We have been servicing medical water treatment equipment for over 40 years and have an experienced nationwide team of technicians qualified to work on your medical water systems. We have a service office within 100 miles of over 70% of the U.S. Medical customers.



Mar Cor Purification 4450 Township Line Road Skippack, PA 19474-1429 Tel: (484) 991-0220 Toll Free: (800) 633-3080 Fax: (484) 991-0230	Mar Cor Purification 14550 28th Avenue North Plymouth, MN 55447 Tel: (484) 991-0220 Toll Free: (800) 633-3080 Fax: (763) 210-3868	Mar Cor Purification 1119 Paulsun Street San Antonio, TX 78219 Tel: (210) 227-3601 Toll Free: (800) 268-5035 Fax: (210) 227-0735	Mar Cor Purification 160 Stedman Street Lowell, MA 01851 Tel: (978) 453-9600 Toll Free: (800) 633-3080 Fax: (978) 453-1223	Mar Cor Purification 6351 Orangethorpe Ave. Buena Park, CA 90620 Tel: (714) 736-9990 Toll Free: (800) 633-3080 Fax: (714) 736-9402
---	--	---	---	---